



POSTERIOR CROWNS

PROCERA®, WOL-CERAM®, LAVA®

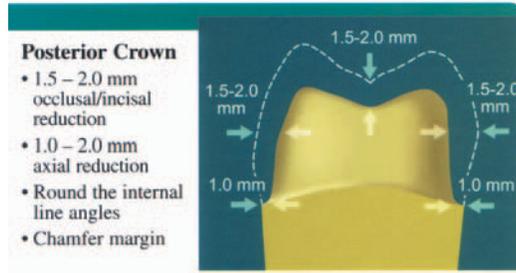


POSTERIOR BRIDGES

PROCERA®, WOL-CERAM®, LAVA®

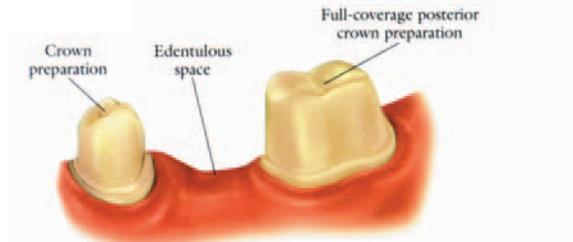


ANTERIOR CROWNS

PROCERA®, WOL-CERAM®, LAVA®

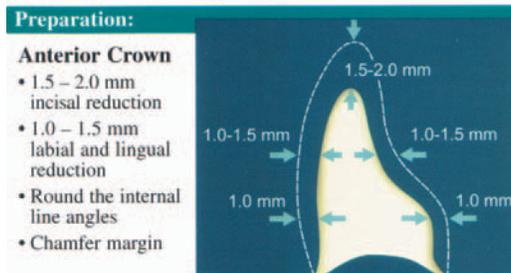

ANTERIOR BRIDGES

PROCERA®, WOL-CERAM®, LAVA®

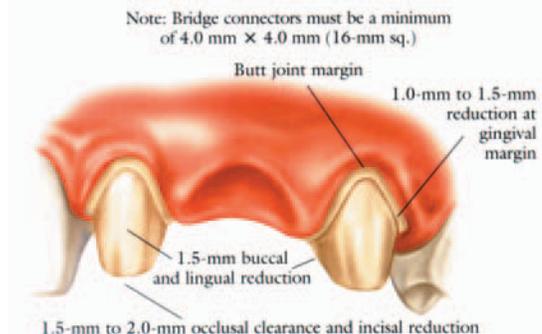

To assure clinical success, the following minimum material thickness is recommended.
All prepared surfaces must be rounded on all metal-free restorations.